



TOYOHASHI UNIVERSITY of TECHNOLOGY

Tempaku-cho, Toyohashi, Aichi, 441-8580 Japan

PHONE: +81-532-44-6577 FAX: +81-532-44-6557

E-mail: press@office.tut.ac.jp

PRESS RELEASE

Source: Toyohashi University of Technology, Japan, Committee for Public Relations

Subject line: Innovative image sensing technology for early diagnosis of diabetes and Alzheimer's disease

(Toyohashi, Japan, 24 September 2014) Researchers at Toyohashi Tech and National Center for Geriatrics and Gerontology in Japan invent an innovative semiconductor-imaging biosensing system for analyzing blood and urine for early diagnosis of diseases including diabetes and Alzheimer's.

This article is featured in the September 2014 issue of the Toyohashi Tech e-Newsletter:

http://www.tut.ac.jp/english/newsletter/tech_overtures/

Professor Kazuaki Sawada and Dr. Takigawa of the National Center for Geriatrics and Gerontology and colleagues at Toyohashi University of Technology have established an easy to use, low-cost, rapid, and high sensitivity semiconductor-imaging based medical diagnostic biosensing system for analyzing blood and urine for early diagnosis of ailments including diabetes and Alzheimer's disease.

The new biosensing technology consists of a semiconductor image sensor ('charge coupled device' developed by Toyohashi University of Technology) that is sensitive to extremely small changes in electric potential, and microbeads on which antigen-antibody reactions take place. This technology will enable monitoring and diagnosis of diseases for which specific markers are known using very small volumes of blood or urine. Specifically, this technology has detected amyloid beta-peptide, an agent responsible for Alzheimer's disease.

Contracting a disease leads to expression of proteins specific to the diseases in the blood. This new technology is used for early diagnosis of diseases by using this specific protein as the antigen and a marker that captures the protein as the antibody and checking their antigen-antibody reaction. Conventional protocols used to monitor antibody-antigen reactions employ fluorescent probes and detection of fluorescence with microscopic cameras. This process is time consuming because of the necessity to measure fluorescence from the probes and cannot be used to detect low concentrations of antigens when the fluorescence intensity is too low to detect optically.

With this technology, an antigen-antibody reaction is used as in conventional methods, but fluorescence is not measured. Instead, this method employs a semiconductor image sensor to detect minute changes in electric potential generated during an antigen-antibody reaction.

The semiconductor image sensor [Fig. 1] consists of 128×128 pixels that independently sense minute changes in electric potential. The detection sensitivity of antigen-antibody reactions was significantly increased by using microbeads [Fig. 2]. The figures of merit of this technology are given in Table 1. Multiple diseases can also be simultaneously diagnosed by placing different antibodies on different sensing pixels out of a total of 16,384 pixels (128×128).

Implementation of the technology will be tested for daily control of lifestyle diseases such as diabetes and in future the technology will be expanded for the early diagnosis of Alzheimer's and Parkinson' diseases.



Acknowledgement

“Extremely early diagnosis technological development project” of the industrial-academic-government collaboration “Knowledge Hub Aichi” project promoted by Aichi Prefecture

Reference:

Akiteru Kono et al, Label free bio image sensor for real time monitoring of potassium ion released from hippocampal slices, *Sensors and Actuators B* 201, 439–443, (2014)

<http://dx.doi.org/10.1016/j.snb.2014.04.019>

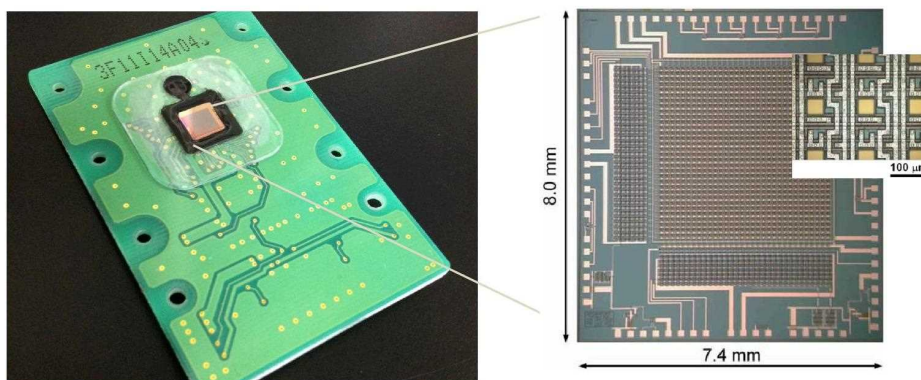


Fig. 1 Semiconductor image sensor (128 pixels × 128 pixels)

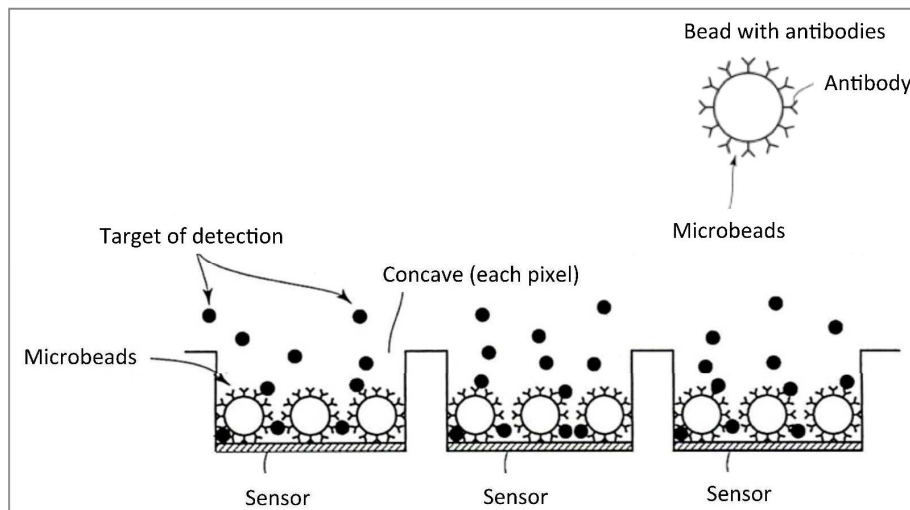


Fig. 2 Schematic illustration of microbeads with antibodies on sensors (Patent application filed)



TOYOHASHI UNIVERSITY of TECHNOLOGY

Tempaku-cho, Toyohashi, Aichi, 441-8580 Japan

PHONE: +81-532-44-6577 FAX: +81-532-44-6557

E-mail: press@office.tut.ac.jp

Item	Measuring time	Sensitivity	Cost (per specimen)	Amount of blood
This technology	About 10 min	0.1-10 pM	100 yen or less	1 drop (0.02ml)
Conventional method (ELISA method)	Several hours	1-100 pM	About 1,000 yen	1-5 ml

Table 1 Advantage of this technology over the conventional method



Kazuaki Sawada

Further information

Toyohashi University of Technology

1-1 Hibarigaoka, Tempaku

Toyohashi, Aichi Prefecture, 441-8580, JAPAN

Inquiries: Committee for Public Relations

E-mail: press@office.tut.ac.jp

About Toyohashi University of Technology:

Founded in 1976 as a National University of Japan, Toyohashi University of Technology is a vibrant modern institute with research activities reflecting the modern era of advanced electronics, engineering, and life sciences.

Website: <http://www.tut.ac.jp/english/>